




COVID-19 / Influenza A+B Antigen Combo Rapid Test





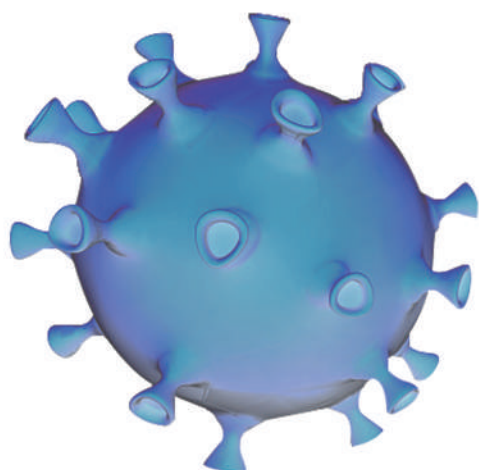

COVID-19 /Influenza A+B Antigen Combo Rapid Test









Clongene has developed the COVID-19/Influenza A+B Antigen Combo Rapid Test. It is a lateral flow immunoassay intended for the qualitative detection of SARS-CoV-2, influenza A and influenza B viral nucleocapsid protein antigens in nasopharyngeal swab from individuals suspected of respiratory viral infection consistent with COVID-19 by their healthcare provider.

Kit Contents

Extraction Reagent Tube	Test Cassette	Work Station	Sterilized Swab
			

Instructions for Use is also included.


Product Features

-  CE Marked
-  Easy to collect samples
-  No equipment required
-  Instant result at 15 minutes
-  Results are clearly visible
-  Suitable for large-scale rapid screening

Test Procedure

1

Insert sterilized swab through the nostril parallel to the palate.

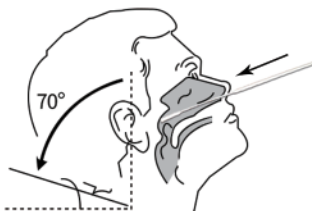


2

Gently rub and roll the swab, and leave swab in place for several seconds to absorb secretions.




3

Slowly remove swab while rotating it.

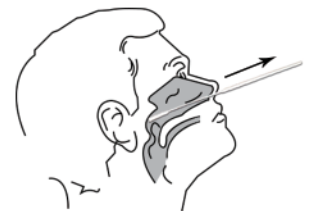


4

Open extraction reagent tube.



5

Insert tube into workstation.




6

Insert swab into tube and rotate swab 5 times.




7

Remove swab and cover the tube.



8

Transfer 3 drops (approximately 100 μ L) to each specimen well (S) of the test cassette.

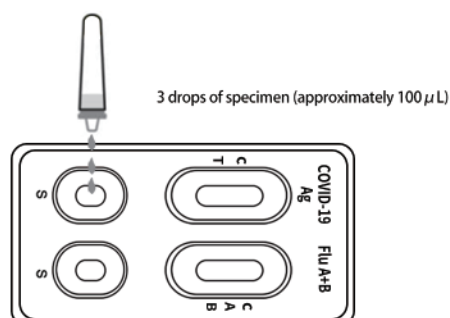




9

Interpret the test results at 15 minutes. Do not read results after 20 minutes.






Interpretation of Results

For COVID-19 Antigen Rapid Test

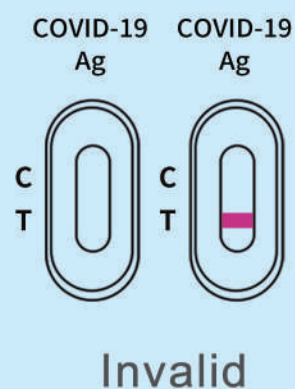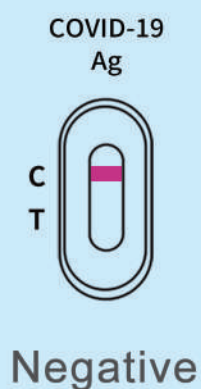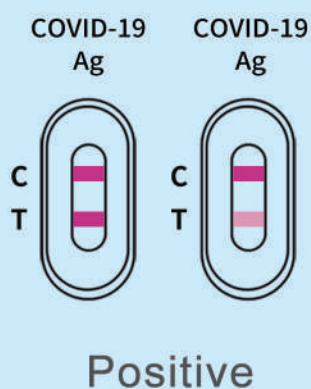

For Influenza A+B Rapid Test

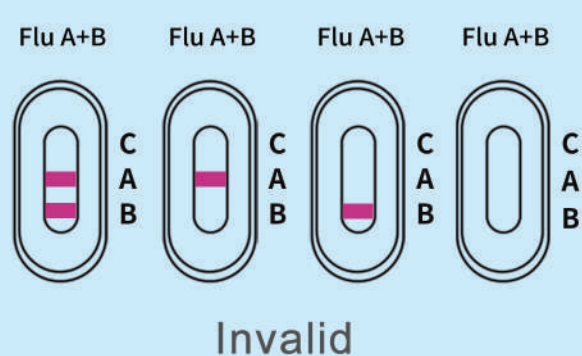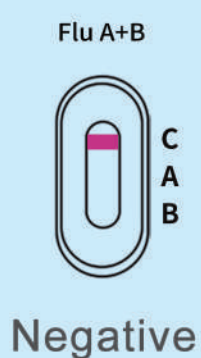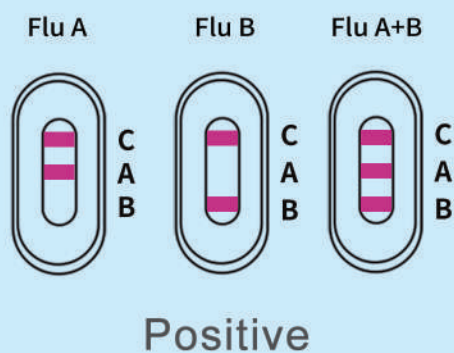

Hangzhou Clongene Biotech Co., Ltd.

Add: No.1 Yichuang Road, Yuhang Sub-district, Yuhang
District, 311121 Hangzhou, China

Tel: +86 (0)571-88617879

400-999-8658

E-mail: marketing@clongene.com

